



# Ultralight Walker Boot (Low Top)

## Instructions For User

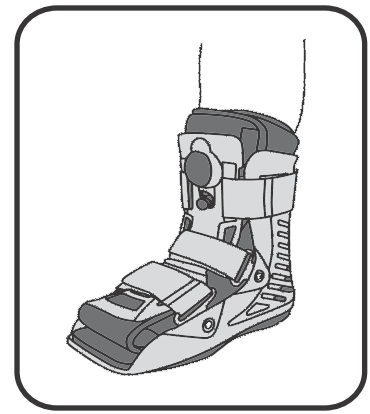


1.

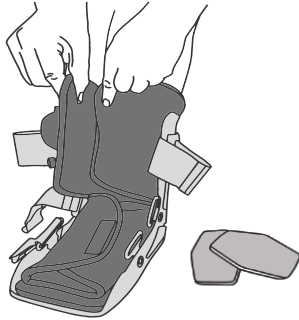


Place foot into walker boot. Wrap liner around foot and leg. Optional: Foam pads may be placed inside liner or between liner and shell for a better fit or greater comfort.

2.

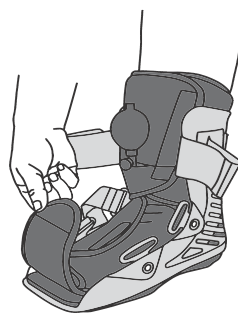


If using the optional toe cover, adjust its positioning if necessary for a proper fit.

3.

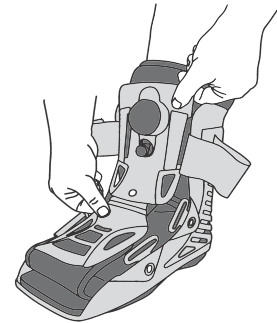


Place front shell over liner and make sure that the air bulb is aligned with the opening.

4.




Thread the straps through the rings to fasten the straps.

5.




Fasten foot, ankle and calf straps. Tighten straps until snug and comfortable.

6.



The walker boot can now be used.

7.



For additional comfort and a better fit, inflate the air liner. For inflation, close the round valve by turning it clockwise and add air by pressing the air bulb until the desired fit is achieved. For deflation, open the round valve by turning it counterclockwise and wait 15 seconds for the air to be released.

**Use and Care:** Hand wash with a mild detergent in luke warm water. Be sure to rinse well because soap residue may cause skin irritation. Air dry.

**Warning:** This device is intended for use only under the guidance of a medical professional. If you experience any pain, swelling, sensation changes, or anything unusual while using this product, consult your medical professional immediately.